

# Radiant Health Saunas Inc.

## Test Summary REPORT

**Model:**  
P-1H, P-3H

**REPORT NUMBER**  
250900041SHA-001

**ISSUE DATE**  
October 30, 2025

**DOCUMENT CONTROL NUMBER**  
TTRFTestsummary\_V1  
© 2018 Intertek



Report no. 250900041SHA-001

**Applicant** : Radiant Health Saunas Inc.  
1333 W Broadway #750, Vancouver, BC V6H 4C1 Canada

**Manufacturer** : [REDACTED]

**Manufacturing site** : [REDACTED]

**Summary**

The equipment complies with the requirements according to the following standard(s) or Specification:

**Electro-Magnetic Radiation Measurement per Manufacturer Requirements**

**PREPARED BY:****REVIEWED BY:**  
Leon Yun  
Project Engineer  
Star Guo  
Reviewer

This report is for the exclusive use of Intertek's Client and is provided pursuant to the agreement between Intertek and its Client. Intertek's responsibility and liability are limited to the terms and conditions of the agreement. Intertek assumes no liability to any party, other than to the Client in accordance with the agreement, for any loss, expense or damage occasioned by the use of this report. Only the Client is authorized to permit copying or distribution of this report and then only in its entirety. Any use of the Intertek name or one of its marks for the sale or advertisement of the tested material, product or service must first be approved in writing by Intertek. The observations and test results in this report are relevant only to the sample tested. This report by itself does not imply that the material, product, or service is or has ever been under an Intertek certification program.

<b>Product Description</b>	: Sauna
<b>Type/Model(s)</b>	: P-1H, P-3H
<b>Rating(s)</b>	: 120VAC, 60Hz; P-1H: 1350W; P-3H: 2200W
<b>Brand name</b>	: Pause
<b>Base testing laboratory</b>	: Intertek Testing Services Shanghai
<b>Test Result: Pass</b>	
Testing on 2 samples: The product covered by this report is a household, indoor use, cord connected IR Sauna room. We tested models P-1H, P-3H at "Max. Time and Max. Temperature" mode on September 18, 2025, and listed the data in this report.	
<b>Electro-Magnetic Radiation Measurement</b>	: Pass

### Revision History

Report No.	Version	Description	Issued Date
250900041SHA-001	Rev. 01	Initial issue of report	October 30, 2025

**Annex I Instrument list**

Electro-Magnetic Radiation Measurement					
Used	Equipment	Manufacturer	Type	Internal no.	Due date
<input checked="" type="checkbox"/>	EMF meter	Narda	BFD-400-1	EC 6898	2026-03-24

## Annex II Test Result

### Electro-Magnetic Radiation Measurement

For model P-1H:

Test Area/ Point	Measured EMF Level ( $\mu\text{T}$ )	Measured EMF Level (milligausse)	Limit (milligausse)	Result
Back point 1	0.0705	0.705	2	Pass
Back point 2	0.0630	0.630	2	Pass
Back point 3	0.0575	0.575	2	Pass
Back point 4	0.0734	0.734	2	Pass
Back point 5	0.0757	0.757	2	Pass
Back point 6	0.0758	0.758	2	Pass
Left point 1	0.0468	0.468	2	Pass
Left point 2	0.0598	0.598	2	Pass
Left point 3	0.0484	0.484	2	Pass
Left point 4	0.0646	0.646	2	Pass
Left point 5	0.0638	0.638	2	Pass
Left point 6	0.0656	0.656	2	Pass
Left point 7	0.0617	0.617	2	Pass
Right point 1	0.0592	0.592	2	Pass
Right point 2	0.0460	0.460	2	Pass
Right point 3	0.0644	0.644	2	Pass
Right point 4	0.0562	0.562	2	Pass
Right point 5	0.0784	0.784	2	Pass
Right point 6	0.0555	0.555	2	Pass
Right point 7	0.0687	0.687	2	Pass
Bench point 1	0.0781	0.781	2	Pass
Vent point 1	0.0930	0.930	2	Pass
Floor point 1	0.0666	0.666	2	Pass
Back panel	0.0913	0.913	2	Pass
Left panel	0.1383	1.383	2	Pass
Right panel	0.0995	0.995	2	Pass
Bench, Vent, Floor panel	0.1108	1.108	2	Pass

For model P-3H:

Test Area/ Point	Measured EMF Level (µT)	Measured EMF Level (milligausse)	Limit (milligausse)	Result
Back A point 1	0.0384	0.384	2	Pass
Back A point 2	0.0448	0.448	2	Pass
Back A point 3	0.0458	0.458	2	Pass
Back A point 4	0.0467	0.467	2	Pass
Back A point 5	0.0446	0.446	2	Pass
Back A point 6	0.0424	0.424	2	Pass
Back B point 1	0.0400	0.400	2	Pass
Back B point 2	0.0490	0.490	2	Pass
Back B point 3	0.0449	0.449	2	Pass
Back B point 4	0.0600	0.600	2	Pass
Back B point 5	0.0545	0.545	2	Pass
Back B point 6	0.0723	0.723	2	Pass
Left point 1	0.0368	0.368	2	Pass
Left point 2	0.0341	0.341	2	Pass
Left point 3	0.0316	0.316	2	Pass
Left point 4	0.0582	0.582	2	Pass
Left point 5	0.0391	0.391	2	Pass
Left point 6	0.0508	0.508	2	Pass
Left point 7	0.0399	0.399	2	Pass
Right point 1	0.0523	0.523	2	Pass
Right point 2	0.0447	0.447	2	Pass
Right point 3	0.0715	0.715	2	Pass
Right point 4	0.0675	0.675	2	Pass
Right point 5	0.0811	0.811	2	Pass
Right point 6	0.0705	0.705	2	Pass
Right point 7	0.0672	0.672	2	Pass
Bench point 1	0.0466	0.466	2	Pass
Bench point 2	0.0727	0.727	2	Pass
Vent point 1	0.0477	0.477	2	Pass
Vent point 2	0.1154	1.154	2	Pass
Floor point 1	0.0455	0.455	2	Pass
Floor point 2	0.0806	0.806	2	Pass
Back A panel	0.1174	1.174	2	Pass
Back B panel	0.1344	1.344	2	Pass
Left panel	0.0966	0.966	2	Pass
Right panel	0.0825	0.825	2	Pass

Bench, Vent, Floor panel	0.1383	1.383	2	Pass
-----------------------------	--------	-------	---	------

**Notes:**

1. The diagram of the test area is shown in the figure below.
2. Background noise: 0.0208  $\mu$ T; Measuring distance: 0 cm.

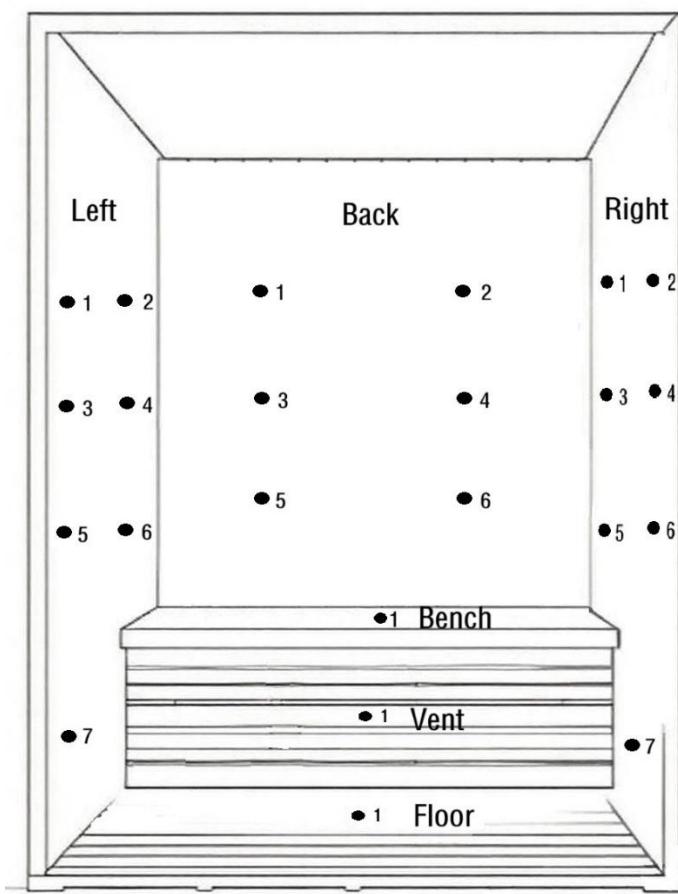


Figure 1: Test Area/ Point for model P-1H


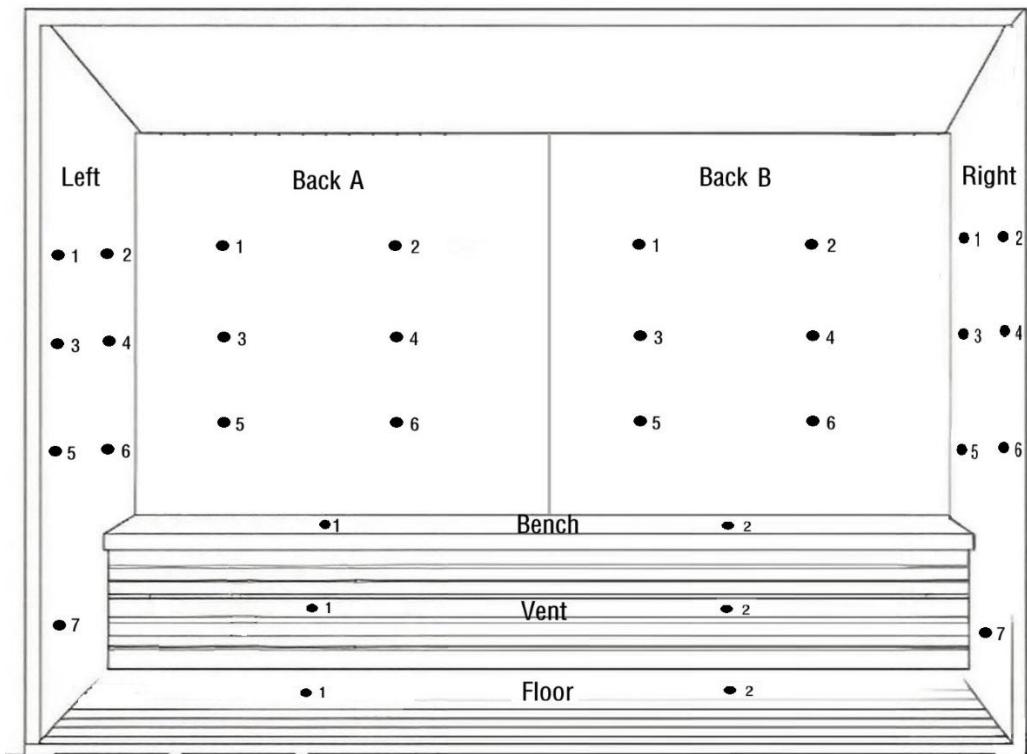


Figure 2: Test Area/ Point for model P-3H

**Annex III: Photograph of Test setup**



**Model P-1H**

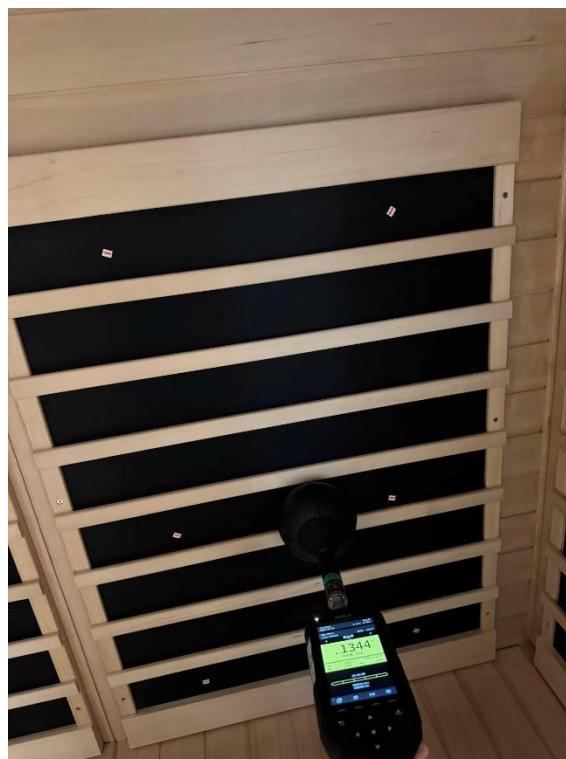

**Model P-3H**

\*\*\*END of the report\*\*\*